


Funnel-to-flask kit for Frac-950

Instructions

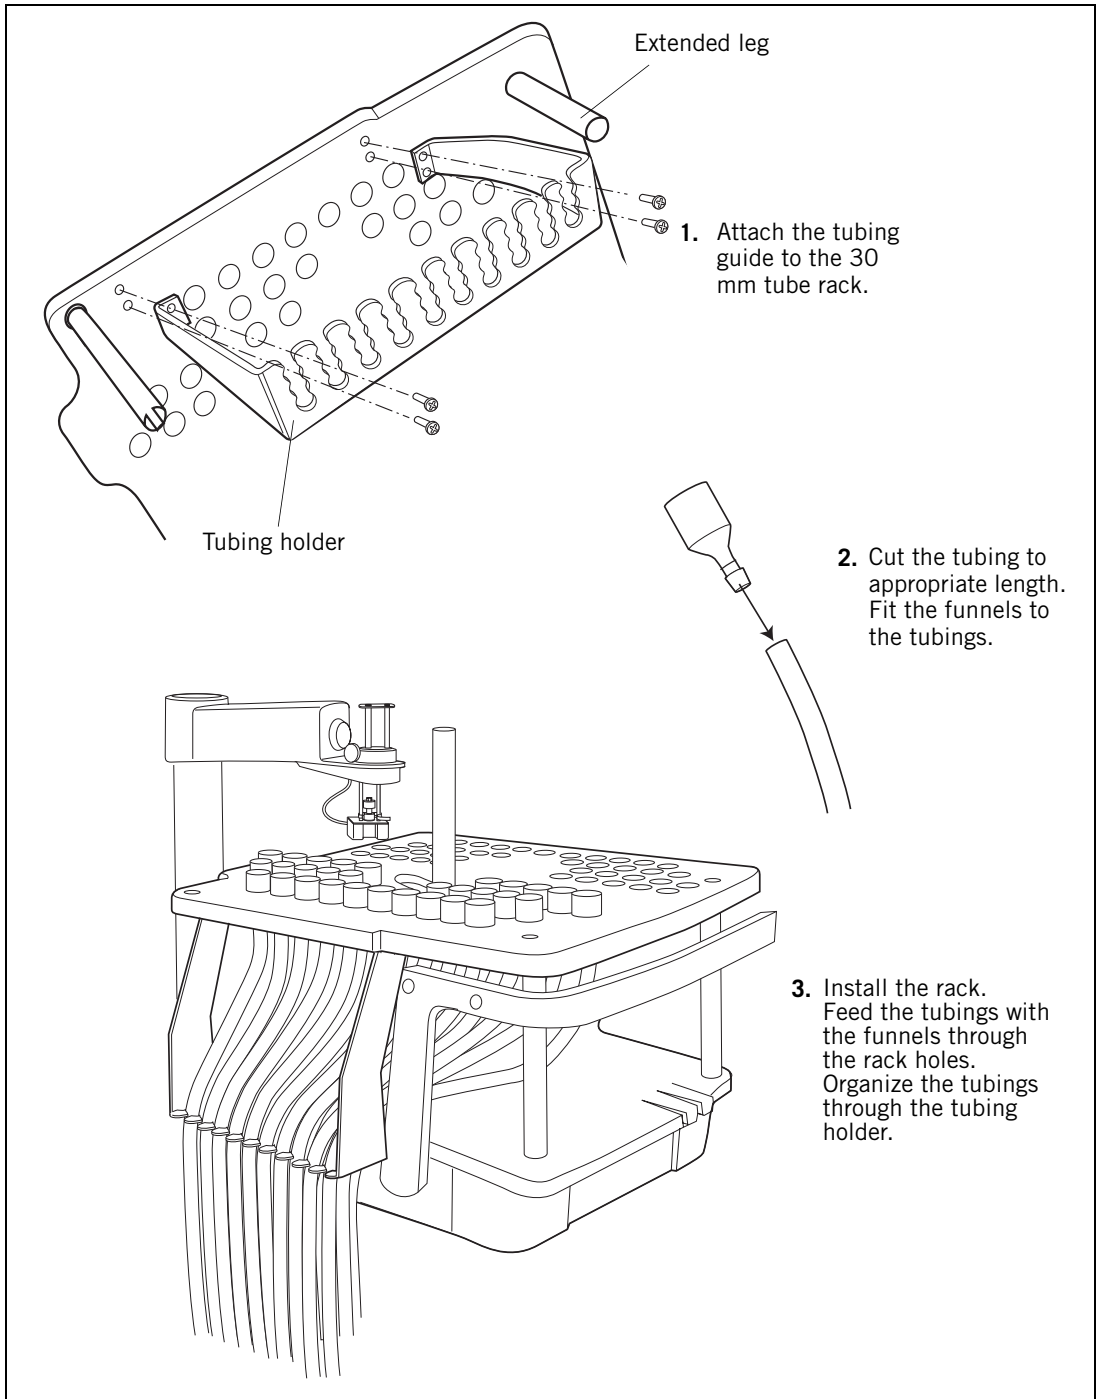

Important user information

Declaration of conformity

The **CE** symbol and corresponding declaration of conformity is valid for the instrument when it is:

- connected to other CE-marked Amersham Biosciences instruments, or
- connected to other products recommended or described in this manual, and
- used in the same state as it was delivered from Amersham Biosciences except for alterations described in this manual.

Terms and Conditions of Sale

Unless otherwise agreed in writing, all goods and services are sold subject to the terms and conditions of sale of the company within the Amersham Biosciences group which supplies them. A copy of these terms and conditions is available on request.

Should you have any comments on this product, we will be pleased to receive them at:

Amersham Biosciences AB
SE-751 84 Uppsala
Sweden

Trademarks

Amersham and Amersham Biosciences are trademarks of Amersham plc.

Office Addresses

Amersham Biosciences AB
SE-751 84 Uppsala
Sweden

Amersham Biosciences UK Limited
Amersham Place, Little Chalfont, Bucks, HP7 9NA
England

Amersham Biosciences Corp.
800 Centennial Avenue
PO Box 1327
Piscataway, NJ 08855
USA

Amersham Biosciences Europe GmbH
Munzinger Strasse 9
D-79111 Freiburg
Germany

Amersham Biosciences KK
Sanken Building
3-25-1 Hyakunincho, Shinjuku-ku
Tokyo 169-0073
Japan

© Amersham Biosciences AB 2002
– All rights reserved